
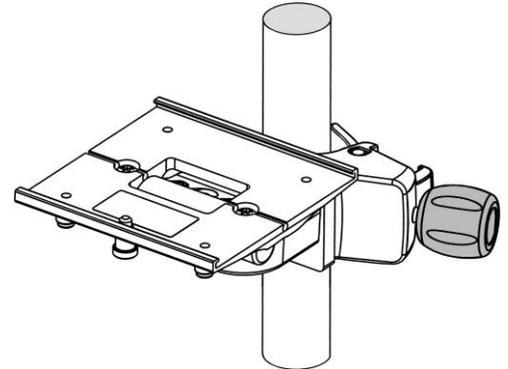


Installation Guide

PRC Clamp with Mounting Plate


For .75" to 1.5" [19 mm-38mm] Diameter Post

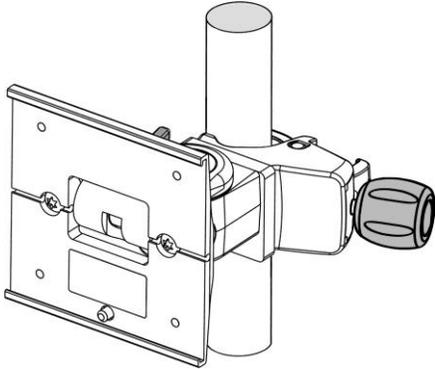

Parts Reference

The following parts and hardware are included with this kit (hardware not shown).

Item #	Description	Qty
1	PRC Clamp with Mounting Plate	1
2	Tilt Lever	1
3	5/32" Hex Wrench	1
4	1/4" Hex Wrench	1

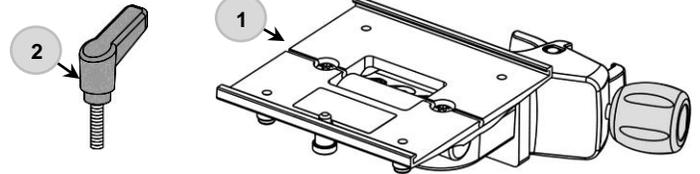


Tools Required:

5/32" and 1/4" hex wrench (supplied)
1/2" Socket Wrench (not supplied)




Warning - The maximum load rating for this product is 10 lbs. [4.5 Kg].

Mounting Clamp on Post (Horizontal Mounting Plate Orientation)

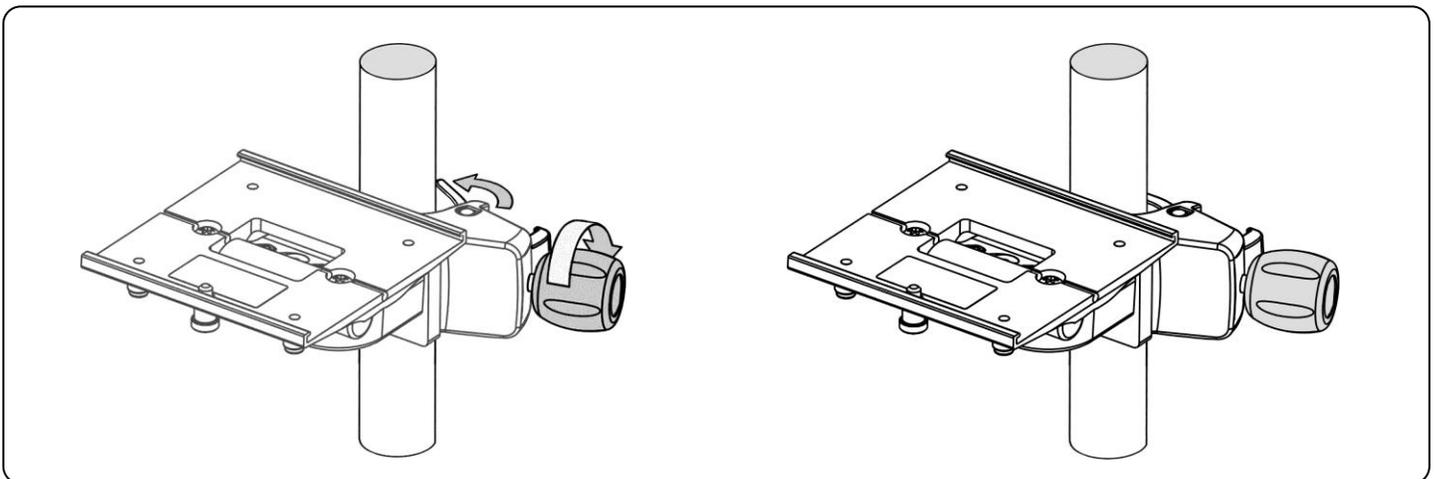


Open Clamp by turning knob counterclockwise (CCW). Position Clamp around post and turn Knob clockwise (CW) to tighten.

Mounting Clamp on Post (Vertical Mounting Plate Orientation)

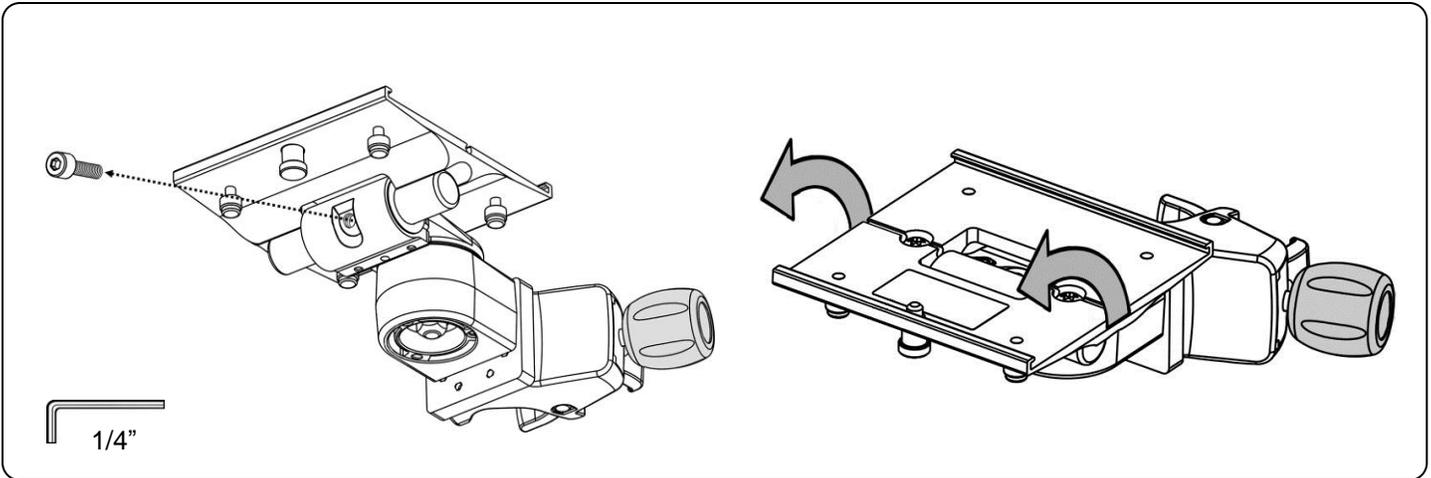

Using a 1/4" hex wrench, remove the tilt limiting screw (above left) and rotate the mounting plate to a vertical orientation.

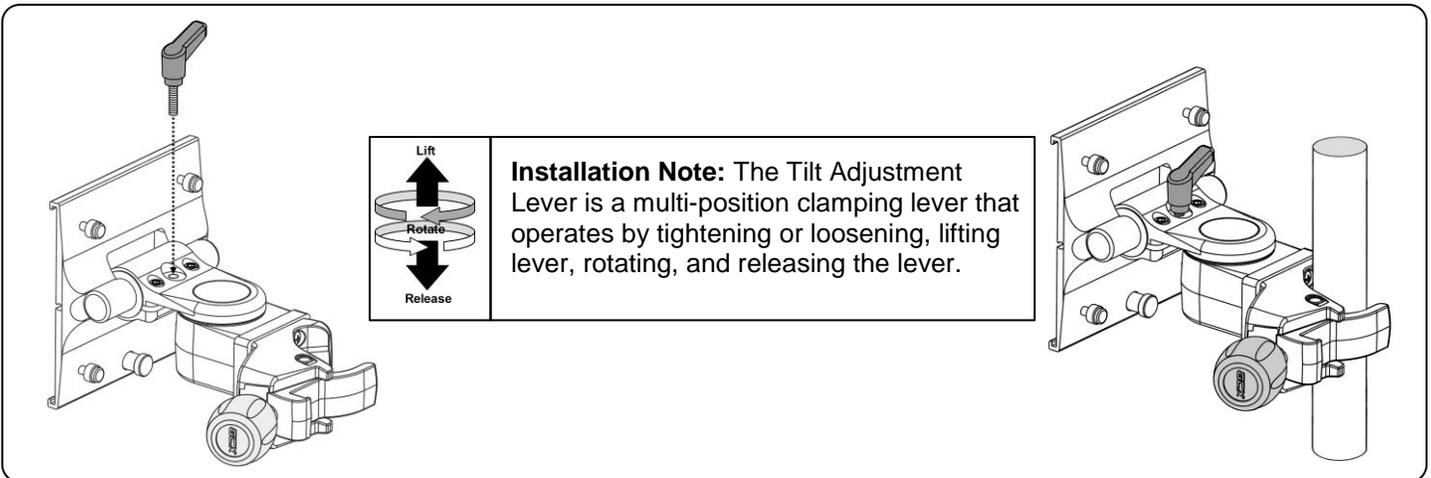

Install Tilt Adjustment Lever (above left). Position Clamp around post and turn Knob clockwise (CW) to secure.


Making Adjustments to the PRC Clamp

Tilt

Adjust tilt by loosening the Tilt Adjustment Lever. Grasp the device and tilt to desired angle. Tighten Tilt Adjustment Lever to lock position.


Tilt Tension

Adjust tilt tension by equally tightening or loosening two (2) Tension Adjustment Screws with the 5/32" hex wrench provided. Once overall tilt tension is set, use Tilt Adjustment Lever to fine tune/lock tilt position.

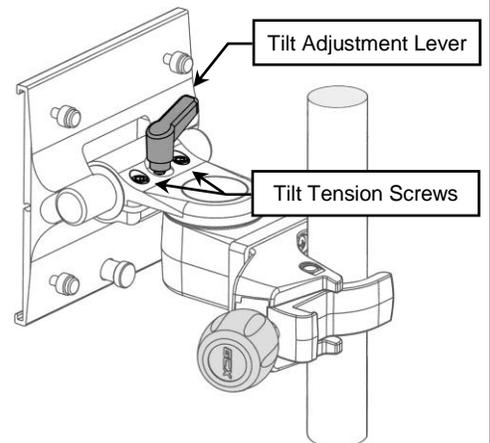

Swivel Adjustment

To adjust the swivel tension, tighten or loosen the Swivel Tension Nut with a 1/2 [13 mm] socket wrench.

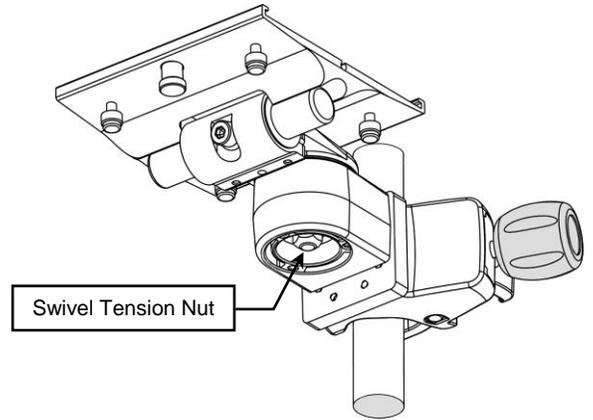

Routine Maintenance

Periodically inspect all fasteners associated with the mounting system. Tighten or adjust fasteners as necessary for optimal operation and safety.

Cleaning the Mounting Assembly

1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone or trichloroethylene.
3. Do not use Steel wool or other abrasive material.
4. Damage caused by the use of unapproved substances or processes will not be warranted. It is recommended that you test any cleaning solution on a small area of the arm that is not visible to verify compatibility.
5. Never submerge or allow liquids to enter the mounting assembly. Wipe any cleaning agents off of the arm immediately, using water dampened cloth. Dry the arm thoroughly after cleaning.

CAUTION: GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted devices or accessory equipment, refer to the specific instructions delivered with those products before installing the arm in the Channel.