

Installation Guide

PTA60 & PTA45 Patient Engagement Tablet Arms with GCX Channel Interface 75mm X 75mm VESA



The arm comes with a USB extension cable – the exact cable included is called out in the specific part number description. Examples: USB A Male to Female Extension Cable or USB C Male to USB A Female Extension Cable

Refer to the label on the Pivot Block to ensure the total weight of the tablet plus tablet enclosure does not exceed the weight rating of the arm --

PTA45 45"/114.3cm Arm: Load Range: 2.6 - 4.0 lbs / 1.2 - 1.8 kg

PTA60 60"/152.4cm Arm: Load Range: 2.6 - 4.0 lbs / 1.2 - 1.8 kg

PE Series
Patient Engagement
Tablet Arm

Load Range:
2.6 - 4.0 lbs / 1.2 - 1.8 kg


GCX
Mounting Solutions
GCX Corporation
3875 Cypress Drive
Petaluma, CA 94954
+1 707.773.1100

CE




Use caution when handling Tablet Arm. Internal gas springs may make the arm suddenly expand.

Parts Reference




1

Using a T10 Torx wrench (supplied), remove the (2) M3 x 10mm Flat Head Torx Machine Screws (FHTMS) and set aside.




Using the 4mm hex wrench (supplied), loosen the (2) handle screws by approximately 3 complete turns. Remove cover and set aside.



Do not remove any screws from opposite side of arm.



2

Secure tablet to the 75 x 75mm VESA mounting pattern in accordance with manufacturers installation guide.

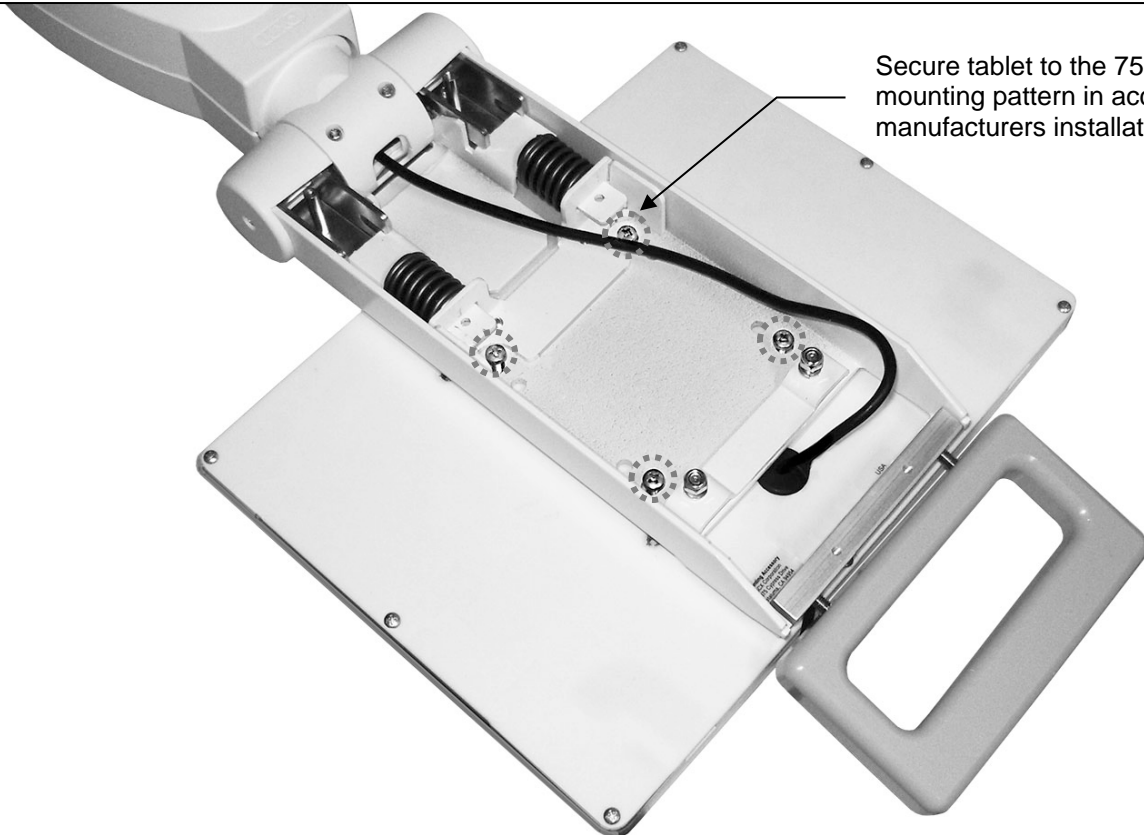


3

Install cover with the (2) M3 x 10mm Torx screws removed in Step 1.

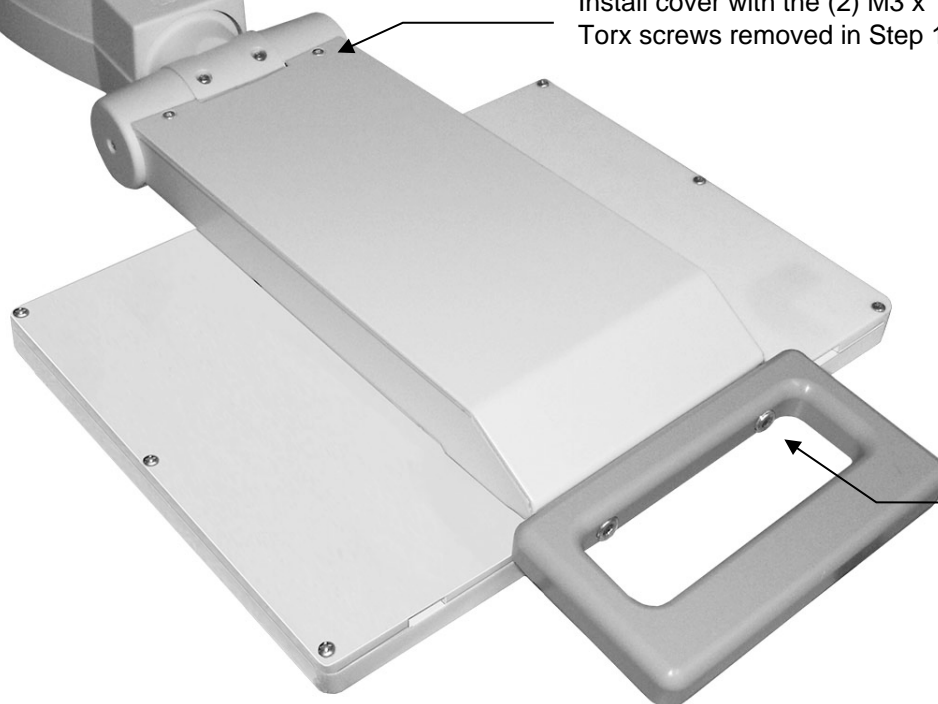


Tighten the (2) handle screws.




4

Guide the slide into top of channel and lower to desired mounting position.

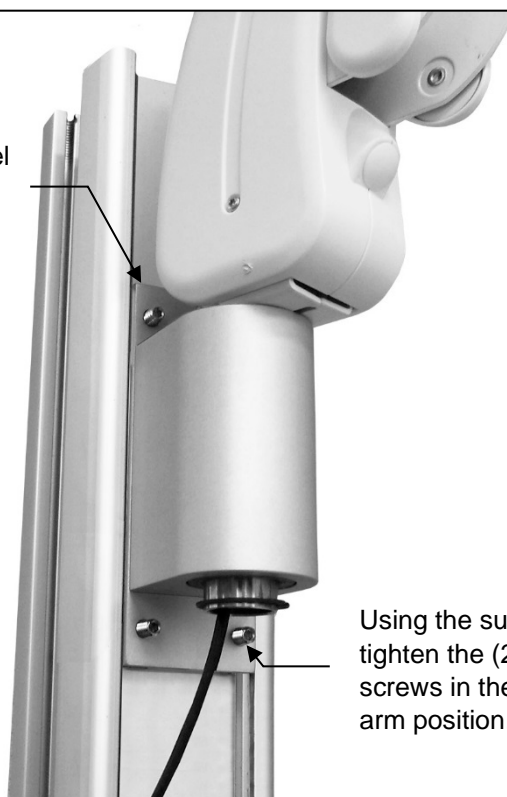

Using the supplied 1/8" hex wrench, tighten the (2) upper and (2) lower set screws in the channel slide to secure arm position.



Routine Maintenance

Periodically inspect all fasteners associated with the mounting system. Tighten or adjust fasteners as necessary for optimal operation and safety.

Cleaning the Mounting Assembly

1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone or trichloroethylene.
3. Do not use Steel wool or other abrasive material.
4. Damage caused by the use of unapproved substances or processes will not be warranted. It is recommended that you test any cleaning solution on a small area of the mounting assembly that is not visible to verify compatibility.
5. Never submerge or allow liquids to enter the mounting assembly. Wipe any cleaning agents off of the assembly immediately, using water dampened cloth. Dry the assembly thoroughly after cleaning.

CAUTION: GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted devices or accessory equipment, refer to the specific instructions delivered with those products.