

# **GCX Mounting Assembly Installation Guide**

Handle for 2" Diameter Post

The purpose of this guide is to describe attachment of Handle to post.

#### **Parts Reference**

The following parts and hardware are included with this installation kit (see photo for parts, hardware not shown):


Item #	Description	Qty
1	Handle	1
2	#10-32 x 9/16" Pan Head Machine Screw (PHMS)	2



Tools Required: Philips screwdriver.

## **Attaching Handle to Post**

1. Fasten Handle to 2" Post with two (2) #10-32 x 9/16" PHMS. Alternately tighten screws until handle does not rotate on Post.

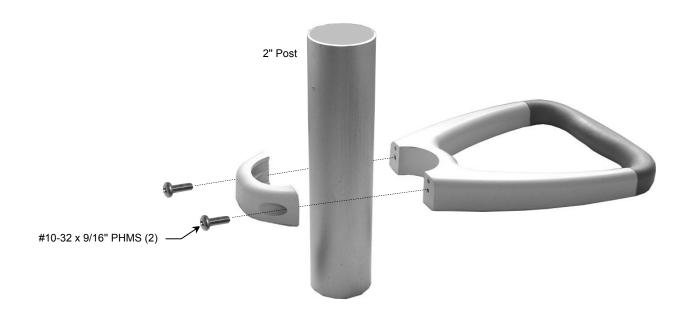

#### **Routine Maintenance**

Periodically inspect all hardware associated with the mounting system. Tighten or adjust as necessary for optimal operation and safety.

### **Cleaning the Mounting Assembly**

- 1. The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).
- 2. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone and trichloroethylene.
- 3. Do not use steel wool or other abrasive material to clean the mounting assembly.
- 4. Damage caused by the use of unapproved substances or processes will not be covered by warranty. We recommend testing of any cleaning solution on a small area of the arm that is not visible to verify compatibility.
- 5. Do not submerge or allow liquids to enter the arm. Wipe any cleaning agents off of the arm immediately using a water-dampened cloth. Dry the arm thoroughly after cleaning.

**CAUTION:** GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted instruments or accessory equipment, refer to the specific instructions delivered with those products.