

3875 Cypress Drive Petaluma, CA 94954 800.228.2555 707.773.1100 Fax 707.773.1180 www.gcx.com INSTRUMENT MOUNTING SYSTEM

# **Installation Guide**

## **Fixed VHM Arm Extension**

The purpose of this guide is to describe installation of Extension and attachment of VHM arm.

#### **Parts Reference**

The following parts and hardware are included with this Extension kit:

Item #	Description	Qty
1	6" Fixed Extension w/5.5" Channel	1
2	1/8" Hex Wrench	1


### **Tools Required**

• 1/8" Hex Wrench (provided)

### Installing Extension

- 1. Guide Arm Extension into channel to desired height.
- 2. Using the 1/8" Hex Wrench, tighten the (4) 1/4-20 Set Screws to secure Extension in place.



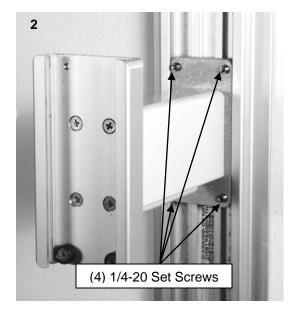



### **VHM Arm Installation**

- 1. Guide VHM onto Arm Extension as shown below
- 2. Using the 1/8" Hex Wrench, tighten Set Screws in the Slide to secure position of the Arm.





### **Routine Maintenance of the Mounting Assembly**

Periodically inspect all hardware associated with the mounting system. Tighten as required for optimal operation and safety.

### **Cleaning the Mounting Assembly**

**1.** The mounting assembly may be cleaned with most mild, non-abrasive solutions commonly used in the hospital environment (e.g. diluted bleach, ammonia, or alcohol solutions).

**2**. The surface finish will be permanently damaged by strong chemicals and solvents such as acetone or trichloroethylene.

3. Do not use Steel wool or other abrasive material.

**4.** Damage caused by the use of unapproved substances or processes will not be warranted. We recommend testing of any cleaning solution on a small area of the arm that is not visible to verify compatibility.

**5.** Never submerge or allow liquids to enter the arm. Wipe any cleaning agents off of the arm immediately using a water dampened cloth. Dry the arm thoroughly after cleaning.

**CAUTION:** GCX makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospital's infection control officer or epidemiologist. To clean or sterilize mounted devices or accessory equipment, refer to the specific instructions delivered with those products.